

RESL CUSTOMER EXPORT CONTROL AGREEMENT

It is the Radiological and Environmental Sciences Laboratory's (RESL) policy to conduct business in accordance with all applicable U.S. export control laws and regulations. It is also RESL's policy that its Customers comply with U.S. export control laws and regulations. Therefore, Customer agrees to the following:

1. Because products, technical data, and technical assistance (i.e., services) provided to Customer by RESL may be subject to U.S. export control laws and regulations, (i) transactions with certain persons and companies and (ii) the export or reexport of certain types and levels of products, technical data, and services are prohibited or restricted.
2. Customer acknowledges that it is responsible for its own compliance with U.S. export control laws and regulations. Customer further agrees that it assumes the responsibility to obtain all necessary U.S. export licenses or other U.S. governmental authorizations, as well as all liability for the failure to do so.
3. Customer acknowledges that export control requirements may change and that the export or reexport of RESL products, technical data, and services without an export license or other appropriate governmental authorization may result in criminal and/or civil liability.
4. The obligations and requirements described herein shall survive the expiration or termination of any agreement or contract between RESL and Customer.

GrW50 Participating Laboratories

Lab Code	Lab Name	Matrix Code
ADEM01	Alabama Department of Environmental Management	GrW
AFOH01	USAFSAM/OEA	GrW
ARGO01	Idaho National Laboratory	GrW
ARPL01	Analytical Support Operations - Radiochemical Processing Lab	GrW
ARSL01	ARS	GrW
ASUK99	AWE (Aldermaston)	GrW
AY1201	Consolidated Nuclear Security, LLC, ACO Laboratory	GrW
CDHS01	California Department of Public Health	GrW
CESL01	Lawrence Livermore National Laboratory - EMRL	GrW
DEHS01	Department of Environmental Health & Safety	GrW
DLEA01	DLE Associates	GrW
ELIW01	Energy Laboratories, Inc.	GrW
ERCL01	Washington State Public Health Laboratories	GrW
ERHD99	National Monitoring Section, Radiation Protection Bureau, Health Canada	GrW
FDHE01	Florida Dept of Health Environmental Laboratory	GrW
GENE01	GEL Laboratories, LLC	GrW
GPCL01	Georgia Power Company Environmental Laboratory	GrW
HCAL01	Lawrence Livermore National Laboratory	GrW
HECR01	SC Dept. Health and Environmental Control Radiological Laboratory	GrW
HPAC99	UKHSA, RCE Glasgow	GrW
HPAL01	Los Alamos National Laboratory	GrW
IEMA01	Illinois Emergency Management Agency Radiochemistry Laboratory	GrW
ISUE01	ISU Environmental Monitoring Laboratory	GrW
LZCA01	ACZ Laboratories, Inc	GrW
MART03	Radioactive Material Analysis Laboratory	GrW
MNDH01	Minnesota Department of Health, Public Health Lab. Division	GrW
NARL01	National Analytical Radiation Environmental Laboratory	GrW
NESI01	BWXT-Radioisotope & Analytical Chemistry Laboratory	GrW
NJDH01	New Jersey Dept. of Health, ECLS	GrW
NSPH01	Nevada State Public Health Laboratory	GrW
ODHL01	Ohio Department of Health Laboratory	GrW
RPSC01	Radiation Protection Service	GrW
SEML01	SRS Environmental Monitoring Laboratory	GrW
SMER01	State of Michigan EGLE Radiological Lab	GrW
STRL01	South Texas Project Radiological Laboratory	GrW
TDHL01	Texas Department of State Health Services Laboratory	GrW
TELE02	Microbac Laboratories Inc. - Northbrook	GrW
TMAO01	EBERLINE Analytical Corporation	GrW
TNUT01	St. Louis USACE FUSRAP Laboratory	GrW
WSHL01	Wisconsin State Laboratory of Hygiene	GrW

Laboratories Not Reporting

Lab Code	Lab Name	Matrix Code
ISUP01	ISU - Department of Physics/Health Physics/EAL	GrW
LOCK03	Advanced Test Reactor (ATR) Complex Radioanalytical Laboratory	GrW
SOUT01	Southwest Research Institute	GrW

Study Reference Values

MAPEP-24-GrW50

Radiological Reference Date: 02/01/2024

Analyte	Ref Value	Ref Unc
Radiological		Units: (Bq/L)
Gross alpha	1.01	0.02
Gross beta	5.57	0.06

Sample Statistical Summary

MAPEP-24-GrW50

Radiological Reference Date: 02/01/2024

Analyte	T(1)	A(2)	Grand(3) Mean	Std Dev	Ref Value	Ref Unc	Acceptance Range
							Units: (Bq/L)
Radiological							
Gross alpha	40	38	0.98	0.21	1.01	0.02	0.30 - 1.72
Gross beta	40	37	5.40	0.72	5.57	0.06	2.79 - 8.36

- Note:**
- (1) T = Total number of laboratories reporting analyte.
 - (2) A = Number of laboratories with 'Acceptable' performance.
 - (3) Mean excludes values derived as total metals and values indicated as "Not Acceptable".

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100

Flag Summary Report

MAPEP-24-GrW50

Radiological

Analyte	A	W	RW	N
Gross alpha	38			2
Gross beta	37			3



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (ADEM01) Alabama Department of Environmental Management
 1350 Coliseum Blvd.
 Montgomery, AL 36110

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.3172	1.01	A		30.4	0.30 - 1.72	0.12469	A
Gross beta	5.994	5.57	A		7.6	2.79 - 8.36	0.15244	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (AFOH01) USAFSAM/OEA
 2510 Fifth Street, Area B
 Wright-Patterson AFB, OH 45433-7913

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.23	1.01	A		21.8	0.30 - 1.72	0.13	A
Gross beta	5.36	5.57	A		-3.8	2.79 - 8.36	0.18	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (ARGO01) Idaho National Laboratory
 INL, Materials and Fuels Complex
 Idaho Falls, ID 83415

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.814	1.01	A		-19.4	0.30 - 1.72	0.080	A
Gross beta	3.16	5.57	A		-43.3	2.79 - 8.36	0.11	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(ARPL01) Analytical Support Operations - Radiochemical Processing Lab

PO Box 999

Richland, WA 99354

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.87	1.01	A		-13.9	0.30 - 1.72	0.12	A
Gross beta	5.3	5.57	A		-4.8	2.79 - 8.36	0.2	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(ARSL01) ARS
 2609 North River Road
 Port Allen, LA 70767

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.047	1.01	A		3.7	0.30 - 1.72	0.131	A
Gross beta	5.273	5.57	A		-5.3	2.79 - 8.36	0.63	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(ASUK99) AWE (Aldermaston)

A38.1 AWE

Reading, Berkshire RG7 4PR

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.2477	1.01	N		-75.5	0.30 - 1.72	0.072	W
Gross beta	6.73	5.57	A		20.8	2.79 - 8.36	1.64	W

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (AY1201) Consolidated Nuclear Security, LLC, ACO Laboratory
 Y12, NSC, Bldg. 9995, Rm 142
 Oak Ridge, TN 37831-8189

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.902	1.01	A		-10.7	0.30 - 1.72	0.086	A
Gross beta	6.03	5.57	A		8.3	2.79 - 8.36	0.22	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (CDHS01) California Department of Public Health
 Drinking Water & Radiation Lab.
 Richmond, CA 94804-6403

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.08	1.01	A		6.9	0.30 - 1.72	0.0659	A
Gross beta	6.13	5.57	A		10.1	2.79 - 8.36	0.0876	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (CESL01) Lawrence Livermore National Laboratory - EMRL
 7000 East Avenue
 Livermore, CA 94551

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.26E+00	1.01	A		24.8	0.30 - 1.72	8.24E-02	A
Gross beta	5.41E+00	5.57	A		-2.9	2.79 - 8.36	7.03E-02	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (DEHS01) Department of Environmental Health & Safety
 North Carolina State Univ.
 Raleigh, NC 27695-8007

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.189	1.01	A		17.7	0.30 - 1.72	0.405	N
Gross beta	4.724	5.57	A		-15.2	2.79 - 8.36	0.75	W

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(DLEA01) DLE Associates

730 Alfred Nobel Drive

Hercules, CA 94547

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.16	1.01	A		14.9	0.30 - 1.72	0.26	W
Gross beta	5.59	5.57	A		0.4	2.79 - 8.36	0.46	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(ELIW01) Energy Laboratories, Inc.

2393 Salt Creek HWY

Casper, Wy 82601

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.6882	1.01	A		-31.9	0.30 - 1.72	0.0777	A
Gross beta	5.328	5.57	A		-4.3	2.79 - 8.36	0.2757	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (ERCL01) Washington State Public Health Laboratories
 1610 N.E. 150th Street
 Shoreline, WA 98155-9701

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.999	1.01	A		-1.1	0.30 - 1.72	0.092	A
Gross beta	5.77	5.57	A		3.6	2.79 - 8.36	0.23	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Laboratory Results For MAPEP-24-GrW50

(ERHD99) National Monitoring Section, Radiation Protection Bureau, Health Canada
 775 Brookfield Road AL6302D1
 Ottawa, Ontario K1A 1C1

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.853	1.01	A		-15.5	0.30 - 1.72	0.172	W
Gross beta	5.699	5.57	A		2.3	2.79 - 8.36	1.364	W

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(FDHE01) Florida Dept of Health Environmental Laboratory
 2100 All Childrens Way
 Orlando, FL 32818-5271

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.86	1.01	A		-14.9	0.30 - 1.72	0.21	W
Gross beta	5.63	5.57	A		1.1	2.79 - 8.36	0.32	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (GENE01) GEL Laboratories, LLC
 2040 Savage Road
 Charleston, SC 29407

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.897	1.01	A		-11.2	0.30 - 1.72	0.117	A
Gross beta	5.01	5.57	A		-10.1	2.79 - 8.36	0.446	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (GPCL01) Georgia Power Company Environmental Laboratory 2480
 Maner Road
 Atlanta, GA 30339

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.92	1.01	A		-8.9	0.30 - 1.72	0.29	N
Gross beta	6.57	5.57	A		18.0	2.79 - 8.36	0.81	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (HCAL01) Lawrence Livermore National Laboratory
 Analytical Services and Instrumentation Analytical Lab
 Livermore, CA 94550

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.83	1.01	A		-17.8	0.30 - 1.72	0.09	A
Gross beta	5.57	5.57	A		0.0	2.79 - 8.36	0.33	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(HECR01) SC Dept. Health and Environmental Control Radiological Laboratory
 8231 Parklane Road
 Columbia, SC 29223

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.24	1.01	A		22.8	0.30 - 1.72	0.239	W
Gross beta	5.67	5.57	A		1.8	2.79 - 8.36	0.240	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (HPAC99) UKHSA, RCE Glasgow
 155 Hardgate Road
 Glasgow, Scotland G51 4LS

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	.848	1.01	A		-16.0	0.30 - 1.72	.089	A
Gross beta	3.87	5.57	A		-30.5	2.79 - 8.36	.17	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Laboratory Results For MAPEP-24-GrW50
 (HPAL01) Los Alamos National Laboratory
 Josh Chandler, z338219 MS G761
 Los Alamos, NM 87545-1663

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1	1.01	A		-1.0	0.30 - 1.72	.1	A
Gross beta	1	5.57	N		-82.0	2.79 - 8.36	.1	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(IEMA01) Illinois Emergency Management Agency Radiochemistry Laboratory
 1301 Knotts St.
 Springfield, IL 62703

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.815	1.01	A		-19.3	0.30 - 1.72	0.043	A
Gross beta	4.856	5.57	A		-12.8	2.79 - 8.36	0.078	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (ISUE01) ISU Environmental Monitoring Laboratory
 785 5th 8th Ave Rm B107
 Pocatello, Idaho 83209

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.63	1.01	A		-37.6	0.30 - 1.72	.03	A
Gross beta	5.92	5.57	A		6.3	2.79 - 8.36	.015	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (LZCA01) ACZ Laboratories, Inc
 2273 Downhill Drive
 Steamboat Springs, CO 80487

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.932	1.01	A		-7.7	0.30 - 1.72	0.189	W
Gross beta	6.35	5.57	A		14.0	2.79 - 8.36	0.266	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (MART03) Radioactive Material Analysis Laboratory
 ORNL
 Oak Ridge, TN 37830

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.16	1.01	A		14.9	0.30 - 1.72	0.12	A
Gross beta	5.87	5.57	A		5.4	2.79 - 8.36	0.21	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(MNDH01) Minnesota Department of Health, Public Health Lab. Division

601 Robert St. N.

St. Paul, MN 55155

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.554	1.01	A		53.9	0.30 - 1.72	0.12728	A
Gross beta	4.38043	5.57	A		-21.4	2.79 - 8.36	0.09065	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(NARL01) National Analytical Radiation Environmental Laboratory
 540 S. Morris Ave.
 Montgomery, AL 36115-2601

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.31	1.01	A		29.7	0.30 - 1.72	0.188	A
Gross beta	5.23	5.57	A		-6.1	2.79 - 8.36	0.295	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (NESI01) BWXT-Radioisotope & Analytical Chemistry Laboratory
 Lynchburg Technology Center
 Lynchburg, VA 24504-5447

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.893	1.01	A		-11.6	0.30 - 1.72	0.049	A
Gross beta	4.95	5.57	A		-11.1	2.79 - 8.36	0.071	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (NJDH01) New Jersey Dept. of Health, ECLS
 3 Schwarzkopf Drive
 Ewing, NJ 08628

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.18	1.01	A		16.8	0.30 - 1.72	0.081	A
Gross beta	5.77	5.57	A		3.6	2.79 - 8.36	0.2	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (NSPH01) Nevada State Public Health Laboratory
 1664 North Virginia Street, MS 328
 Reno, NV 89557

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.999	1.01	A		-1.1	0.30 - 1.72	0.083	A
Gross beta	5.21	5.57	A		-6.5	2.79 - 8.36	0.109	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (ODHL01) Ohio Department of Health Laboratory
 8995 E Main Street
 Reynoldsburg, OH 43068

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.67	1.01	A		-33.7	0.30 - 1.72	0.09	A
Gross beta	5.66	5.57	A		1.6	2.79 - 8.36	0.23	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (RPSC01) Radiation Protection Service
 O. Ministry of Labour, Immigration, Training & Skills Development
 Mississauga, Ontario L4V 1W8

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.75	1.01	A		-25.7	0.30 - 1.72	0.32	N
Gross beta	4.17	5.57	A		-25.1	2.79 - 8.36	1.33	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (SEML01) SRS Environmental Monitoring Laboratory
 Bldg 735-B
 Aiken, SC 29808

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.867	1.01	A		-14.2	0.30 - 1.72	0.103	A
Gross beta	5.642	5.57	A		1.3	2.79 - 8.36	0.192	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (SMER01) State of Michigan EGLE Radiological Lab
 815 Filley St.
 Lansing, MI 48906

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	3.12	1.01	N		208.9	0.30 - 1.72	0.6	W
Gross beta	18.1	5.57	N		225.0	2.79 - 8.36	0.9	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (STRL01) South Texas Project Radiological Laboratory
 12090 FM 521
 Wadsworth, Texas 77483

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.906	1.01	A		-10.3	0.30 - 1.72	0.033	A
Gross beta	21.57	5.57	N		287.3	2.79 - 8.36	0.18	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50

(TDHL01) Texas Department of State Health Services Laboratory
 1100 W 49th Street
 Austin, TX 78756

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.984	1.01	A		-2.6	0.30 - 1.72	0.068	A
Gross beta	4.97	5.57	A		-10.8	2.79 - 8.36	0.12	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (TELE02) Microbac Laboratories Inc. - Northbrook
 700 Landwehr Road
 Northbrook, IL 60062-

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.641	1.01	A		-36.5	0.30 - 1.72	0.048	A
Gross beta	4.71	5.57	A		-15.4	2.79 - 8.36	0.08	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (TMAO01) EBERLINE Analytical Corporation
 601 A SCARBORO RD
 OAK RIDGE, TN 37830-

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	0.7791	1.01	A		-22.9	0.30 - 1.72	0.111	A
Gross beta	6.003	5.57	A		7.8	2.79 - 8.36	0.197	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (TNUT01) St. Louis USACE FUSRAP Laboratory
 112 James S McDonnell Blvd
 HAZELWOOD, MO 63042

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.10	1.01	A		8.9	0.30 - 1.72	0.167	W
Gross beta	5.64	5.57	A		1.3	2.79 - 8.36	0.154	A

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$

ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100



Department of Energy RESL - 1955 Fremont Ave, MS4149 - Idaho Falls, ID 83415

Laboratory Results For MAPEP-24-GrW50
 (WSHL01) Wisconsin State Laboratory of Hygiene
 2601 Agriculture Drive
 Madison, WI 53718

Radiological							Units: (Bq/L)	
Analyte	Result	Ref Value	Flag	Notes	Bias (%)	Acceptance Range	Unc Value	Unc Flag
Gross alpha	1.2	1.01	A		18.8	0.30 - 1.72	0.073	A
Gross beta	5.48	5.57	A		-1.6	2.79 - 8.36	0.093	N

Radiological Reference Date: February 1, 2024

Gross Alpha Flags:

A = Result acceptable, Bias $\leq \pm 70\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 70\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Gross Beta Flags:

A = Result acceptable, Bias $\leq \pm 50\%$ with a statistically positive result at two standard deviations (Result/Uncertainty > 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, does not include zero).

N = Result not acceptable, Bias $> \pm 50\%$ or the reported result is not statistically positive at two standard deviations (Result/Uncertainty ≤ 2 , i.e., the range encompassing the result, plus or minus the total uncertainty at two standard deviations, includes zero).

Uncertainty Flags:

NOT ACCEPTABLE.....RP $< 2\%$

ACCEPTABLE..... $2\% \leq RP \leq 15\%$


ACCEPTABLE WITH WARNING..... $15\% < RP \leq 30\%$

NOT ACCEPTABLE.....RP $> 30\%$

Relative Precision (RP) = (Reported Uncertainty / Reported Result) x 100

Gross alpha

MAPEP-24-GrW50

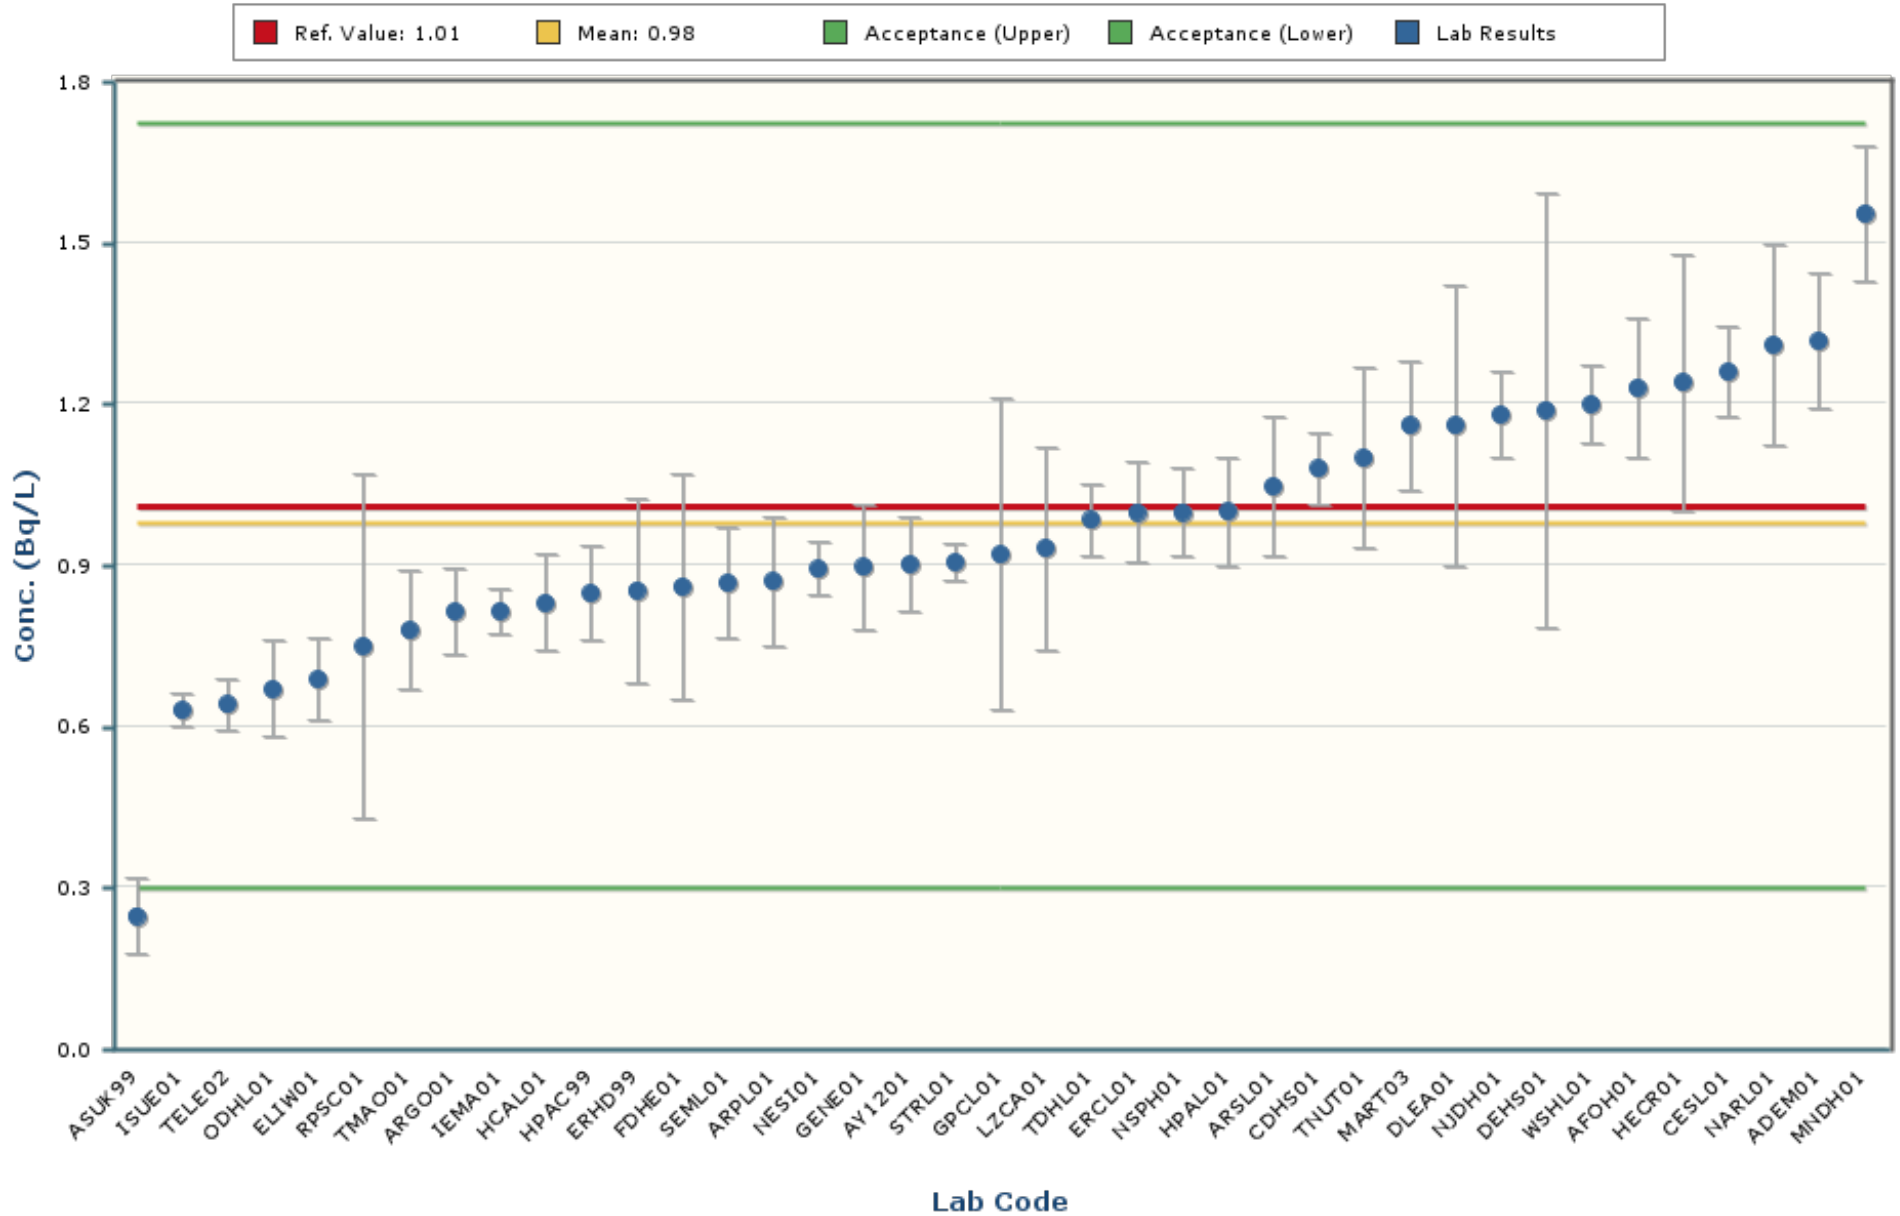


Notes:

The chart shows only data points with values between -0.08 and 2.05 (± 5 Standard Deviations).

Gross beta


MAPEP-24-GrW50

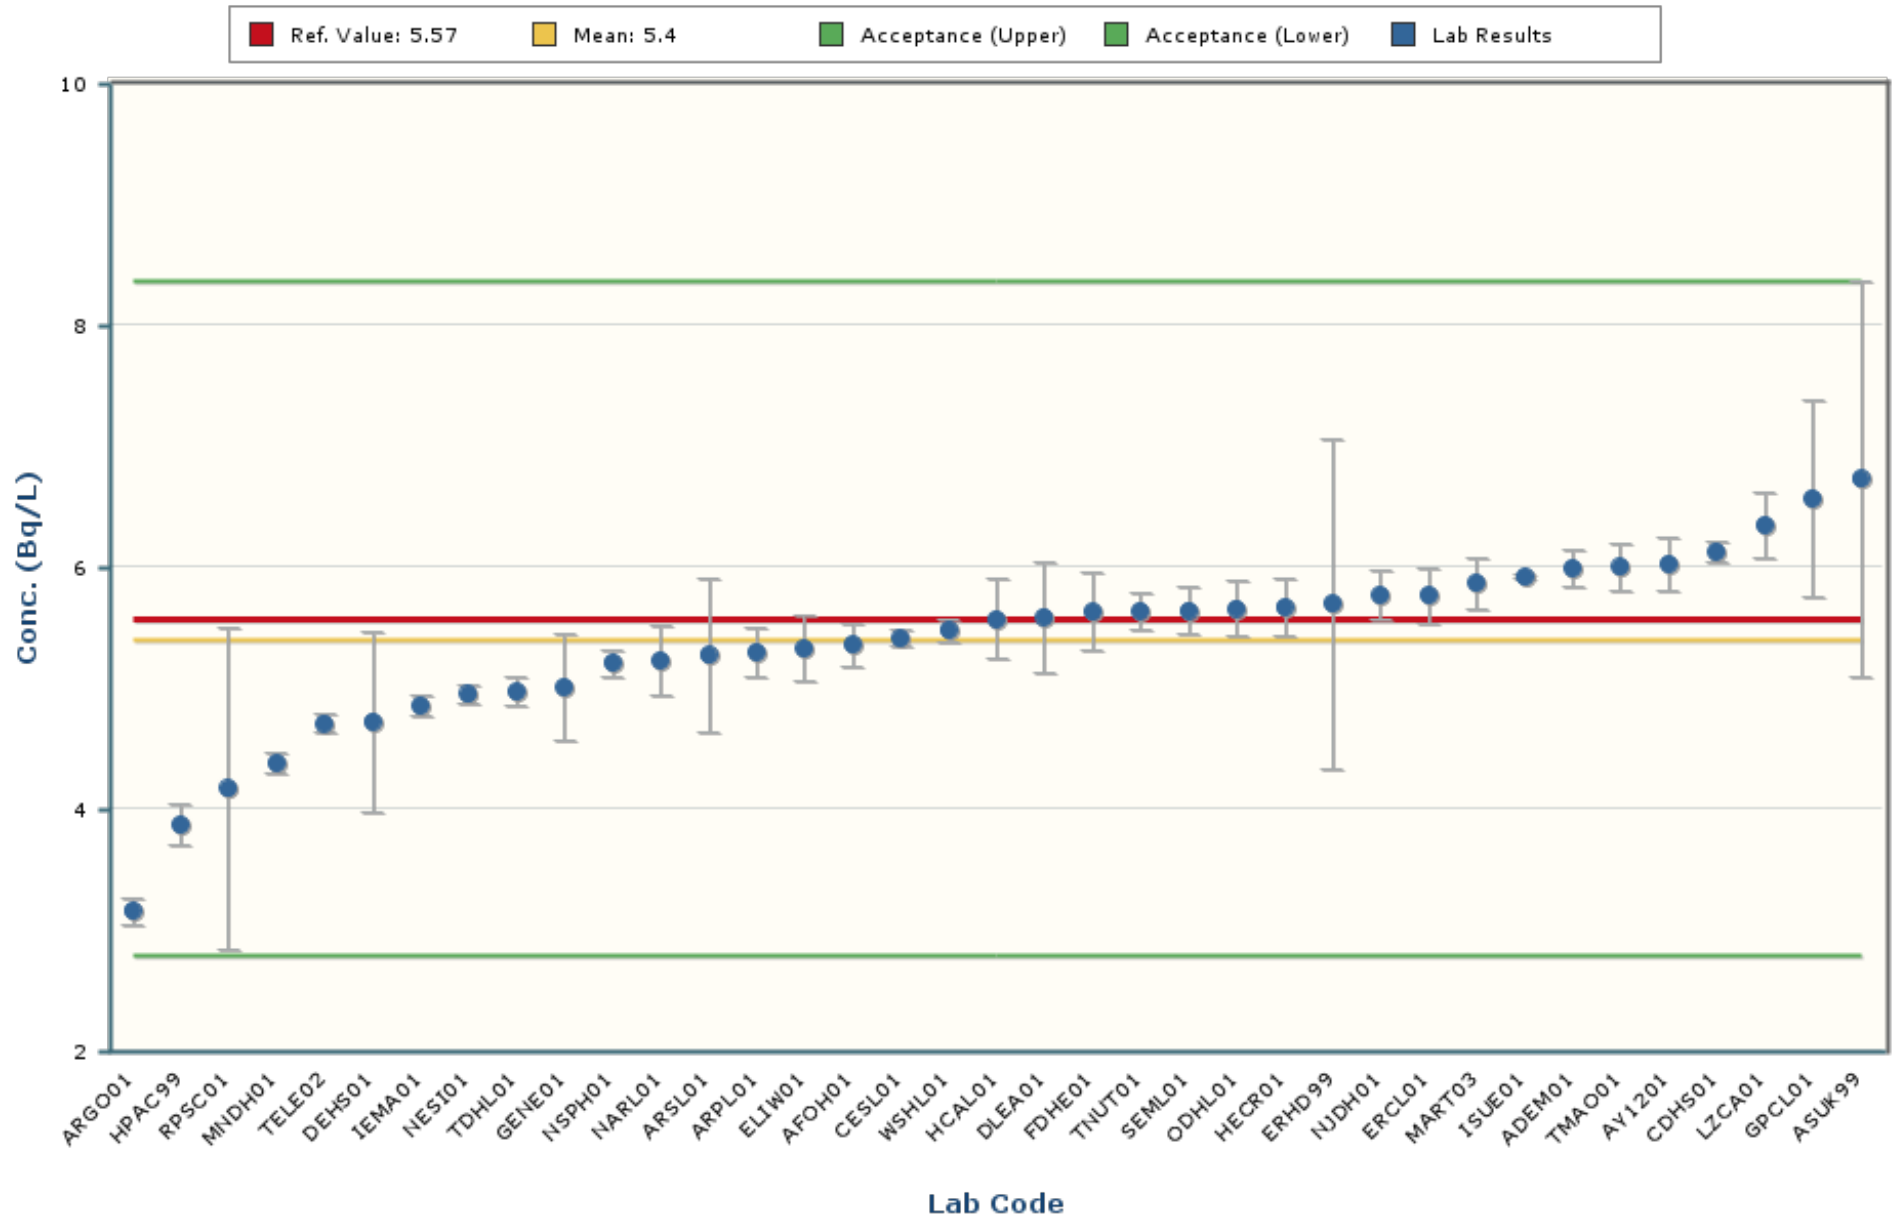

Notes:

The chart shows only data points with values between 1.79 and 9.00 (± 5 Standard Deviations).

The intent of the distribution graphs contained within this report is to graphically demonstrate to users how % Bias data within the current MAPEP Series appears when examined by matrix, by analyte, by method of sample preparation or by method of detection. Biases greater than +/- 100% have been screened from the data. The box plot of the bias data points and the mean visually illustrate the breadth of the distribution and where potential outliers in the distribution might lie. The statistics for the distribution plot are provided adjacent to the Bias plot. In some cases, N becomes very small and thus developed statistics may not accurately reflect estimates of the population if N were a significantly larger value.

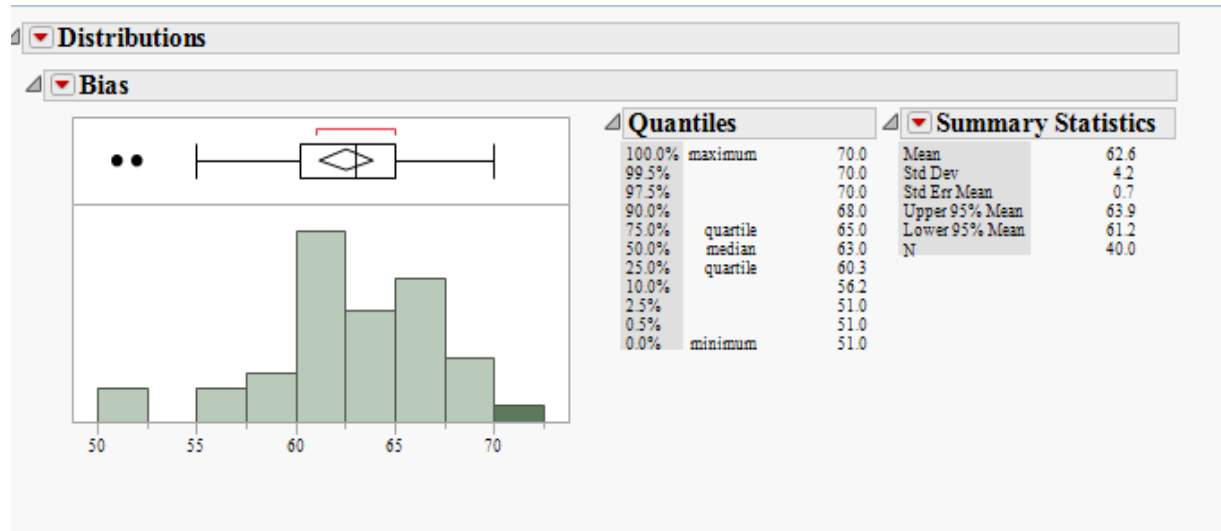


Outlier Box Plot

The BLACK small vertical line inside the small rectangle at the top of the data distribution graph is the median of the population of the bias shown for that analyte in the matrix. The confidence diamond contains the mean and the upper and lower 95% of the mean. If you drew a line through the middle of the diamond, you would have the mean. The top and bottom points of the diamond represent the upper and lower 95% of the mean. The ends of the box represent the 25th and 75th quantiles, also expressed as 1st and 3rd quartile. The difference between the 1st and 3rd quartiles is called the interquartile range. Each box has lines that extend from each end, sometimes called whiskers. The whiskers extend from the ends of the box to the outermost data point that falls within the distances computed as follows:

3rd quartile + 1.5*(interquartile range)

1st quartile - 1.5*(interquartile range)

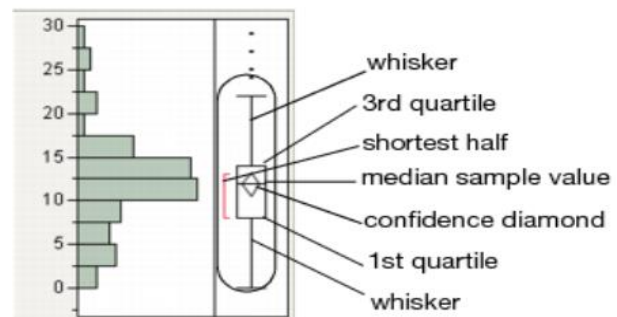


If the data points do not reach the computed ranges, then the whiskers are determined by the upper and lower data point values (not including outliers). The bracket outside of the box identifies the *shortest half*, which is the most dense 50% of the observations (Rousseuw and Leroy 1987).

GrW50 Distribution by Detection Method

Distributions Analyte_Detection=Gross alpha Gas Flow Proportional Counter

Bias

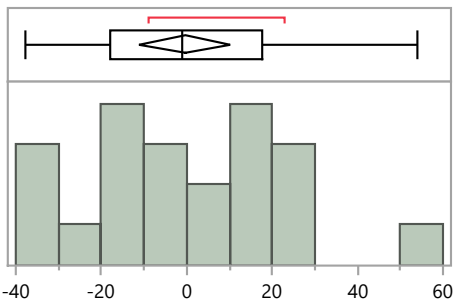

Quantiles


100.0%	maximum	53.9
99.5%		53.9
97.5%		53.9
90.0%		24.4
75.0%	quartile	17.8
50.0%	median	-1.1
25.0%	quartile	-17.7
10.0%		-35.6
2.5%		-37.6
0.5%		-37.6
0.0%	minimum	-37.6

Summary Statistics

Mean	-0.4
Std Dev	23.7
Std Err Mean	5.2
Upper 95% Mean	10.3
Lower 95% Mean	-11.2
N	21.0

Distributions Analyte_Detection=Gross alpha Gross Alpha/Beta - 2 pi gas flow proportional counter

Bias

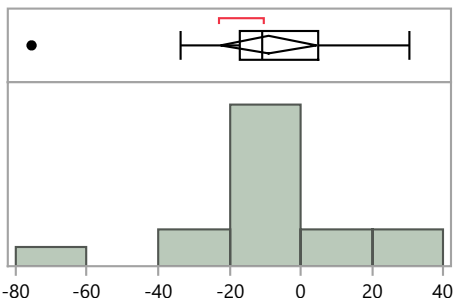

Quantiles


100.0%	maximum	30.4
99.5%		30.4
97.5%		30.4
90.0%		29.9
75.0%	quartile	4.9
50.0%	median	-11.0
25.0%	quartile	-17.2
10.0%		-46.2
2.5%		-75.5
0.5%		-75.5
0.0%	minimum	-75.5

Summary Statistics

Mean	-9.1
Std Dev	25.2
Std Err Mean	6.3
Upper 95% Mean	4.3
Lower 95% Mean	-22.5
N	16.0

Distributions Analyte_Detection=Gross alpha Liquid Scintillation Counter

Bias

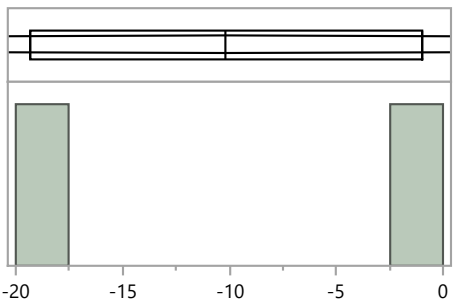

Quantiles

100.0%	maximum	-1.0
99.5%		-1.0
97.5%		-1.0
90.0%		-1.0
75.0%	quartile	-1.0
50.0%	median	-10.2
25.0%	quartile	-19.3
10.0%		-19.3
2.5%		-19.3
0.5%		-19.3
0.0%	minimum	-19.3


Summary Statistics

Mean	-10.2
Std Dev	12.9
Std Err Mean	9.2
Upper 95% Mean	106.1
Lower 95% Mean	-126.4
N	2.0

GrW50 Distribution by Detection Method

Distributions Analyte_Detection=Gross beta Gas Flow Proportional Counter

Bias

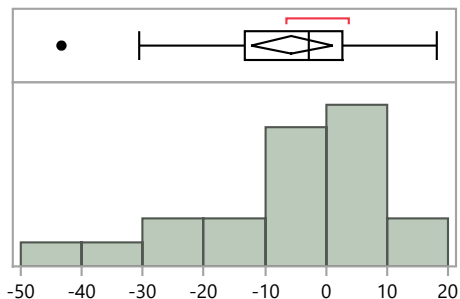

Quantiles


100.0%	maximum	18.0
99.5%		18.0
97.5%		18.0
90.0%		12.5
75.0%	quartile	2.7
50.0%	median	-2.9
25.0%	quartile	-13.3
10.0%		-29.4
2.5%		-43.3
0.5%		-43.3
0.0%	minimum	-43.3

Summary Statistics

Mean	-5.7
Std Dev	14.7
Std Err Mean	3.2
Upper 95% Mean	1.0
Lower 95% Mean	-12.3
N	21.0

Distributions Analyte_Detection=Gross beta Gross Alpha/Beta - 2 pi gas flow proportional counter

Bias

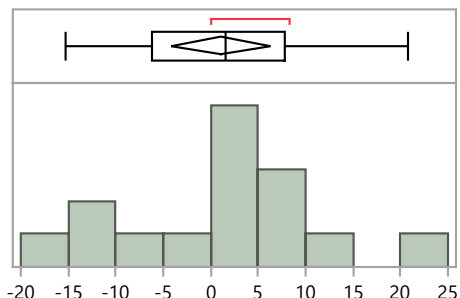

Quantiles


100.0%	maximum	20.8
99.5%		20.8
97.5%		20.8
90.0%		14.4
75.0%	quartile	7.8
50.0%	median	1.6
25.0%	quartile	-6.1
10.0%		-12.6
2.5%		-15.2
0.5%		-15.2
0.0%	minimum	-15.2

Summary Statistics

Mean	1.1
Std Dev	9.4
Std Err Mean	2.4
Upper 95% Mean	6.3
Lower 95% Mean	-4.1
N	15.0

Distributions Analyte_Detection=Gross beta Liquid Scintillation Counter

Bias

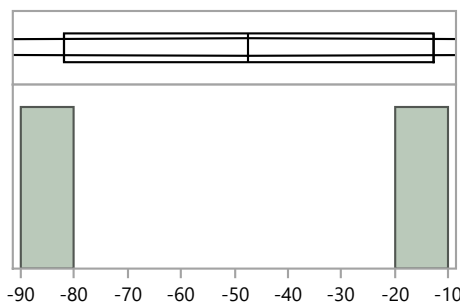

Quantiles

100.0%	maximum	-12.8
99.5%		-12.8
97.5%		-12.8
90.0%		-12.8
75.0%	quartile	-12.8
50.0%	median	-47.4
25.0%	quartile	-82.0
10.0%		-82.0
2.5%		-82.0
0.5%		-82.0
0.0%	minimum	-82.0


Summary Statistics

Mean	-47.4
Std Dev	48.9
Std Err Mean	34.6
Upper 95% Mean	392.2
Lower 95% Mean	-487.0
N	2.0

GrW50 Distribution by Preparation Method

Distributions Analyte_Method=Gross alpha Coprecipitation, acidified

Bias

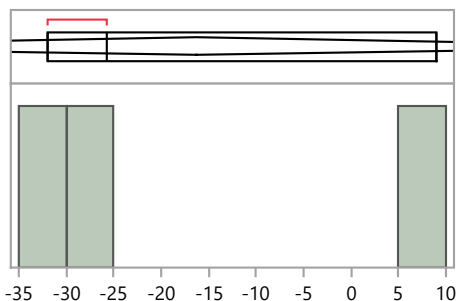

Quantiles


100.0%	maximum	8.9
99.5%		8.9
97.5%		8.9
90.0%		8.9
75.0%	quartile	8.9
50.0%	median	-25.7
25.0%	quartile	-31.9
10.0%		-31.9
2.5%		-31.9
0.5%		-31.9
0.0%	minimum	-31.9

Summary Statistics

Mean	-16.2
Std Dev	22.0
Std Err Mean	12.7
Upper 95% Mean	38.4
Lower 95% Mean	-70.8
N	3.0

Distributions Analyte_Method=Gross alpha Coprecipitation, straight

Bias

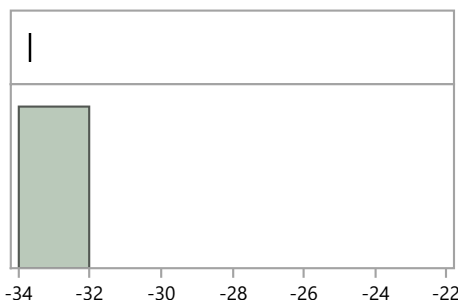

Quantiles


100.0%	maximum	-33.7
99.5%		-33.7
97.5%		-33.7
90.0%		-33.7
75.0%	quartile	-33.7
50.0%	median	-33.7
25.0%	quartile	-33.7
10.0%		-33.7
2.5%		-33.7
0.5%		-33.7
0.0%	minimum	-33.7

Summary Statistics

Mean	-33.7
Std Dev	.
Std Err Mean	.
Upper 95% Mean	.
Lower 95% Mean	.
N	1.0

Distributions Analyte_Method=Gross alpha EPA 900, Radioactivity, Gross Alpha/Beta Screening, 600/4-80-032

Bias

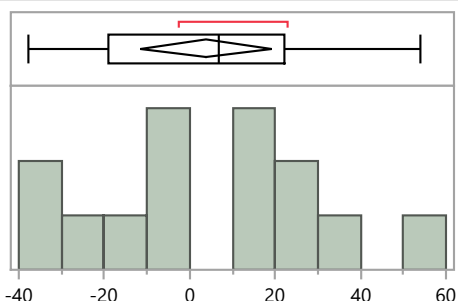

Quantiles

100.0%	maximum	53.9
99.5%		53.9
97.5%		53.9
90.0%		42.2
75.0%	quartile	22.1
50.0%	median	6.9
25.0%	quartile	-19.1
10.0%		-37.1
2.5%		-37.6
0.5%		-37.6
0.0%	minimum	-37.6


Summary Statistics

Mean	3.8
Std Dev	26.5
Std Err Mean	7.1
Upper 95% Mean	19.1
Lower 95% Mean	-11.5
N	14.0

GrW50 Distribution by Preparation Method

Distributions Analyte_Method=Gross alpha Evaporation, acidified

Bias

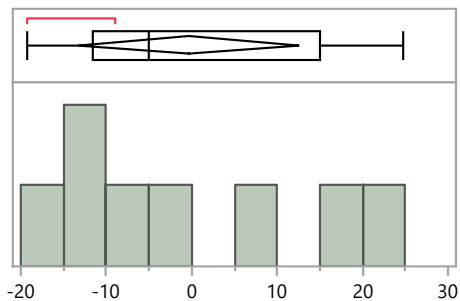


Quantiles		
100.0%	maximum	24.8
99.5%		24.8
97.5%		24.8
90.0%		24.8
75.0%	quartile	15.0
50.0%	median	-5.0
25.0%	quartile	-11.5
10.0%		-19.3
2.5%		-19.3
0.5%		-19.3
0.0%	minimum	-19.3

Summary Statistics	
Mean	-0.3
Std Dev	15.5
Std Err Mean	5.5
Upper 95% Mean	12.6
Lower 95% Mean	-13.3
N	8.0

Distributions Analyte_Method=Gross alpha Evaporation, straight

Bias

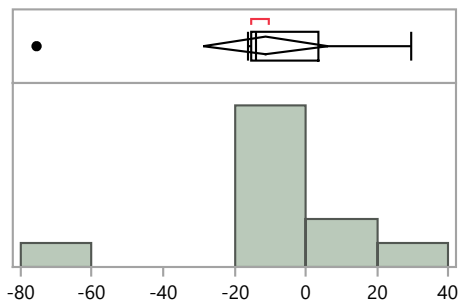


Quantiles		
100.0%	maximum	29.7
99.5%		29.7
97.5%		29.7
90.0%		26.7
75.0%	quartile	3.7
50.0%	median	-13.9
25.0%	quartile	-15.5
10.0%		-63.6
2.5%		-75.5
0.5%		-75.5
0.0%	minimum	-75.5

Summary Statistics	
Mean	-11.2
Std Dev	26.0
Std Err Mean	7.9
Upper 95% Mean	6.3
Lower 95% Mean	-28.7
N	11.0

Distributions Analyte_Method=Gross alpha No preparation - analyzed as received

Bias

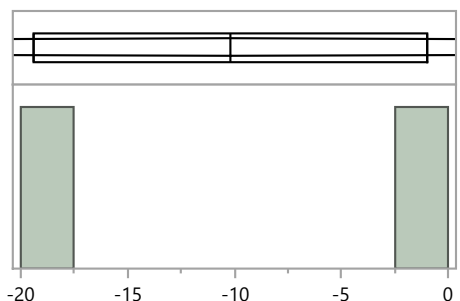


Quantiles		
100.0%	maximum	-1.0
99.5%		-1.0
97.5%		-1.0
90.0%		-1.0
75.0%	quartile	-1.0
50.0%	median	-10.2
25.0%	quartile	-19.4
10.0%		-19.4
2.5%		-19.4
0.5%		-19.4
0.0%	minimum	-19.4

Summary Statistics	
Mean	-10.2
Std Dev	13.0
Std Err Mean	9.2
Upper 95% Mean	106.7
Lower 95% Mean	-127.1
N	2.0

GrW50 Distribution by Preparation Method

Distributions Analyte_Method=Gross beta Coprecipitation, acidified

Bias

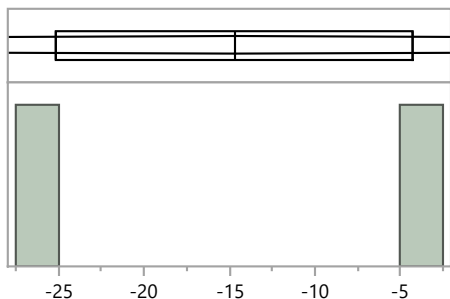

Quantiles


100.0%	maximum	-4.3
99.5%		-4.3
97.5%		-4.3
90.0%		-4.3
75.0%	quartile	-4.3
50.0%	median	-14.7
25.0%	quartile	-25.1
10.0%		-25.1
2.5%		-25.1
0.5%		-25.1
0.0%	minimum	-25.1

Summary Statistics

Mean	-14.7
Std Dev	14.7
Std Err Mean	10.4
Upper 95% Mean	117.4
Lower 95% Mean	-146.8
N	2.0

Distributions Analyte_Method=Gross beta EPA 900, Radioactivity, Gross Alpha/Beta Screening, 600/4-80-032

Bias

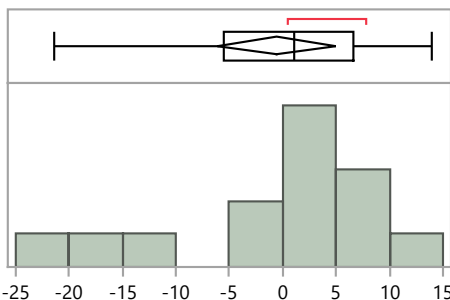

Quantiles


100.0%	maximum	14.0
99.5%		14.0
97.5%		14.0
90.0%		10.9
75.0%	quartile	6.6
50.0%	median	1.1
25.0%	quartile	-5.6
10.0%		-18.4
2.5%		-21.4
0.5%		-21.4
0.0%	minimum	-21.4

Summary Statistics

Mean	-0.6
Std Dev	9.6
Std Err Mean	2.6
Upper 95% Mean	5.0
Lower 95% Mean	-6.1
N	14.0

Distributions Analyte_Method=Gross beta Evaporation, acidified

Bias

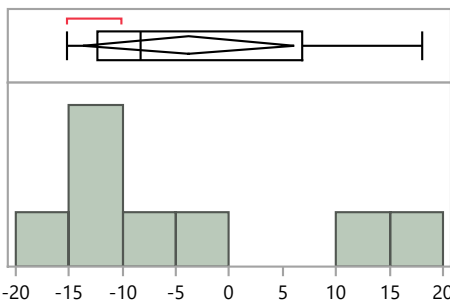

Quantiles

100.0%	maximum	18.0
99.5%		18.0
97.5%		18.0
90.0%		18.0
75.0%	quartile	6.9
50.0%	median	-8.3
25.0%	quartile	-12.4
10.0%		-15.2
2.5%		-15.2
0.5%		-15.2
0.0%	minimum	-15.2


Summary Statistics

Mean	-3.8
Std Dev	11.8
Std Err Mean	4.2
Upper 95% Mean	6.1
Lower 95% Mean	-13.7
N	8.0

GrW50 Distribution by Preparation Method

Distributions Analyte_Method=Gross beta Evaporation, straight

Bias

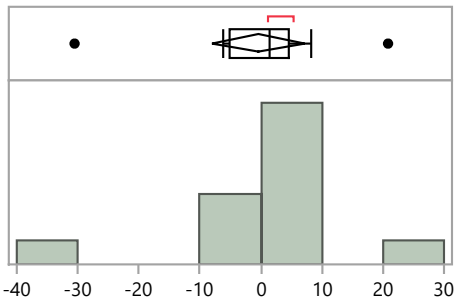


Quantiles	
100.0%	maximum 20.8
99.5%	20.8
97.5%	20.8
90.0%	17.1
75.0%	quartile 4.6
50.0%	median 1.3
25.0%	quartile -5.2
10.0%	-23.2
2.5%	-30.5
0.5%	-30.5
0.0%	minimum -30.5

Summary Statistics	
Mean	-0.4
Std Dev	11.9
Std Err Mean	3.4
Upper 95% Mean	7.2
Lower 95% Mean	-7.9
N	12.0

Distributions Analyte_Method=Gross beta No preparation - analyzed as received

Bias

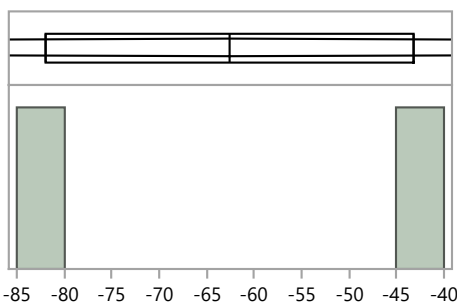

Quantiles	
100.0%	maximum -43.3
99.5%	-43.3
97.5%	-43.3
90.0%	-43.3
75.0%	quartile -43.3
50.0%	median -62.7
25.0%	quartile -82.0
10.0%	-82.0
2.5%	-82.0
0.5%	-82.0
0.0%	minimum -82.0

Summary Statistics	
Mean	-62.7
Std Dev	27.4
Std Err Mean	19.4
Upper 95% Mean	183.2
Lower 95% Mean	-308.5
N	2.0